2617 - Pull String Bed Monitor with Magnet



What's in the box?


2617 Pull String Bed Monitor with Magnet


Fixing Strap


9V Battery


QuickStart User Guide

Compatible & Optional Accessories


Nurse Call Cables: 2643, 2646, 2493, 2461, 2460

cura¹
10 Gray Street, Kilkenny South Australia 5009
www.cura1.com


1300-12-CARE (2273)

UM-06c


All our products are supplied with a full warranty and are guaranteed to be free from defects in material and workmanship.

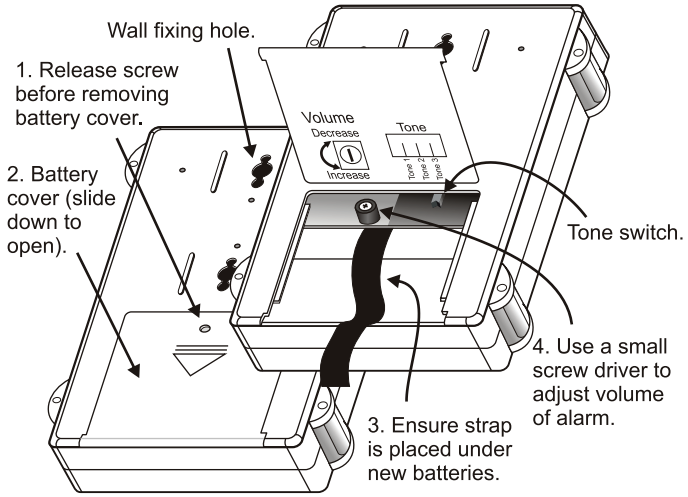


Unscrew the battery cover.
Insert 9V battery in position.
Before screwing back the cover, you may want to adjust the alarm volume and tone.

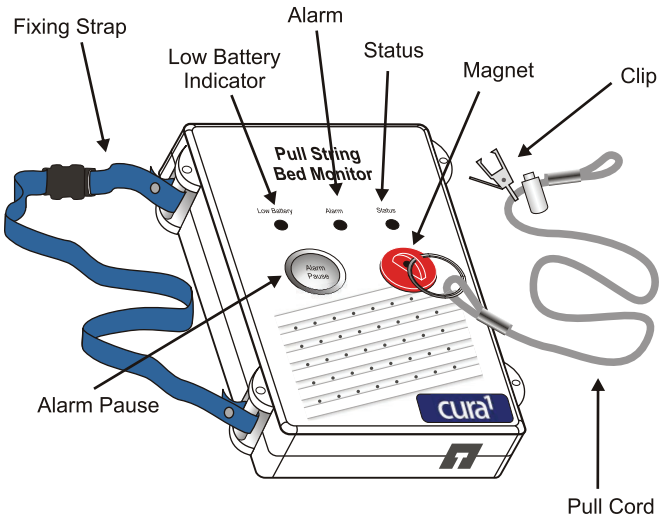

Monitor must be tested prior to use.

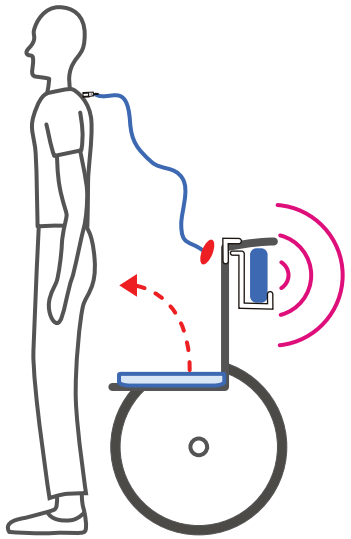

Fix Pull String Monitor to chair or bed (optional mounting holders are available). Attach pull string to patient.

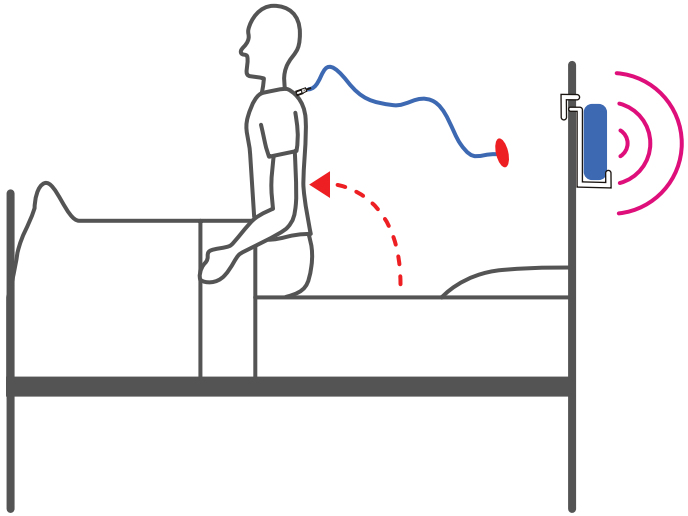

Alarm sounds when the magnetic pull string cord end is disconnected from the monitor.