cura1.com
1300 12 2273

2614 SafeTime Falls Monitor

Optional Accessories (Sold Seperately)

2623 SafeTime Bed Pad 1 Year

2622 Safetime Bed Pad 90 Days

2621 SafeTime Chair Pad 1 Year

2620 SafeTime Chair Pad 90 Days

2642 Caregiver Reset Key

2626 Premium Bed Pad

2628 Premium Chair Pad

2633 Premium Heavy Duty Floor Mat

2636 Easy Release Seatbelt

2406 Plug Pack 6V Power Adaptor

2643 Nurse call cable

2641 Soft Plastic Cover



Do NOT fold pads or mats when in transit or storage.





Keep pads & mats flat at all times




Do not immerse or wash pads or mats under running water. Use a damp cloth (1/1000 bleach solution) & wipe clean. Dry all spills on mats immediately.

All our products are supplied with a full warranty and are guaranteed to be free from defects in material and workmanship

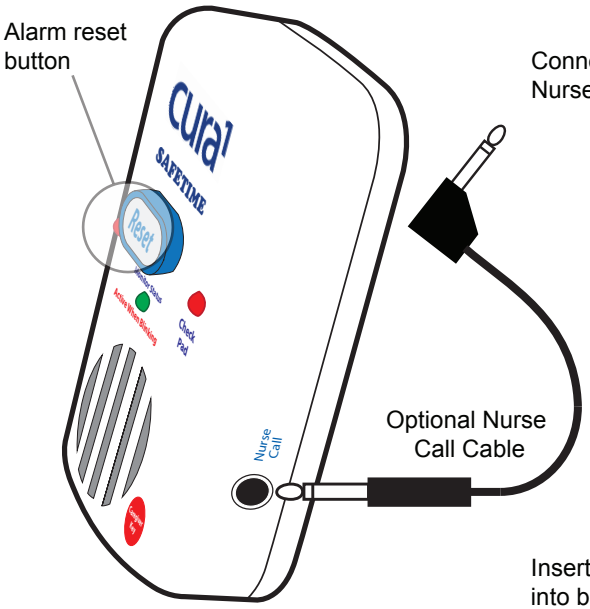

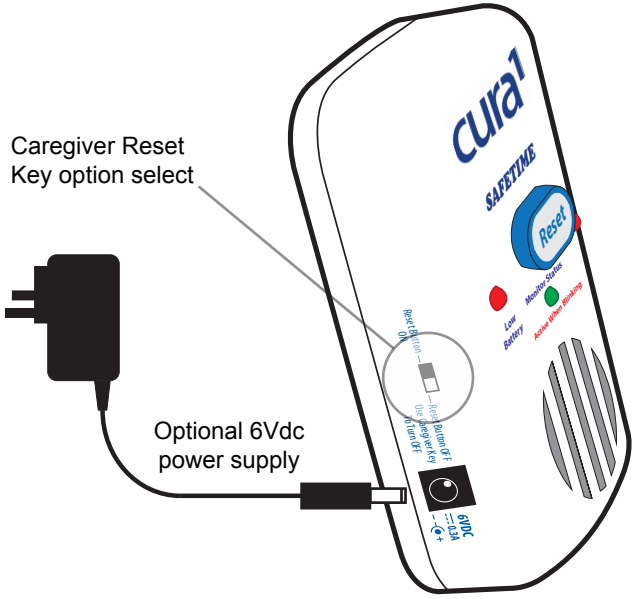

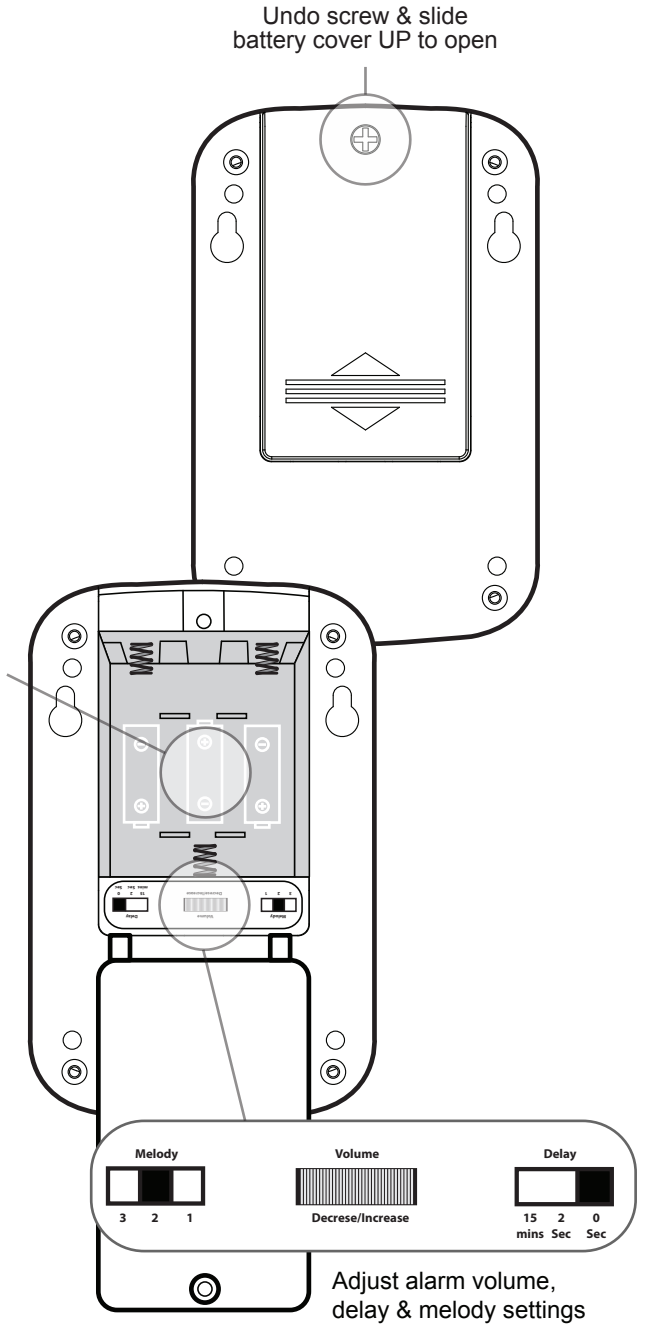

UM-002C

QUICK START GUIDE

2614 SafeTime Falls Monitor

Step 1

Insert 3 x AA Battery.


Step 2

Connect pad or floor mat to monitor

& test prior to using.

Step 3

Place pad on mattress or position mat on floor.

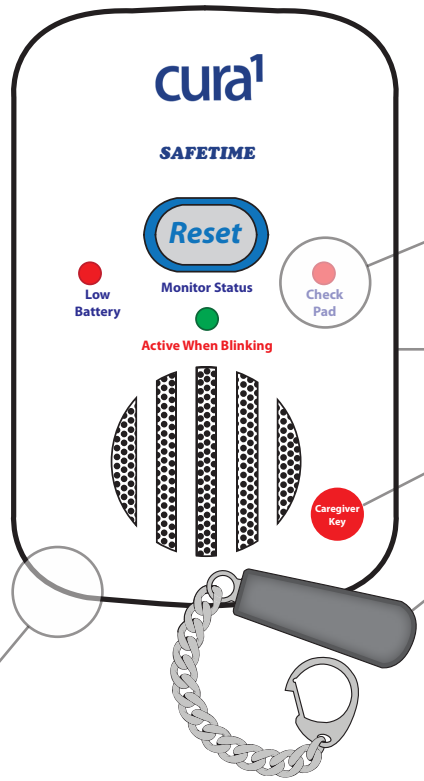

1

Back View


Insert 3 X AA batteries into battery compartment

Check Pad light will illuminate & Monitor will beep when SafeTime Bed or Chair Pad expires

Caregiver Reset Key application point


Caregiver Reset Key

Open battery cover

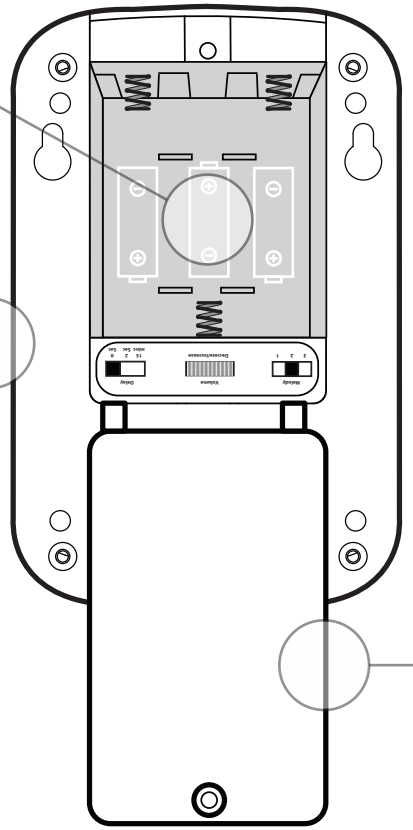

2

Bottom View

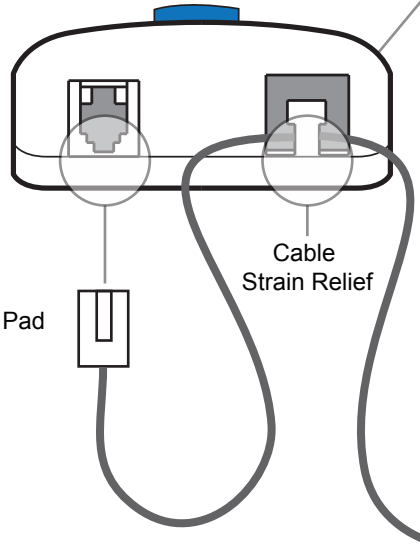


Connection to Bed / Chair Pad or Floor Mat

Cable Strain Relief


SafeTime Bed or Chair Pad

Premium Pads & Mats can also be used with SafeTime Falls Monitor but will not the have SafeTime features

3

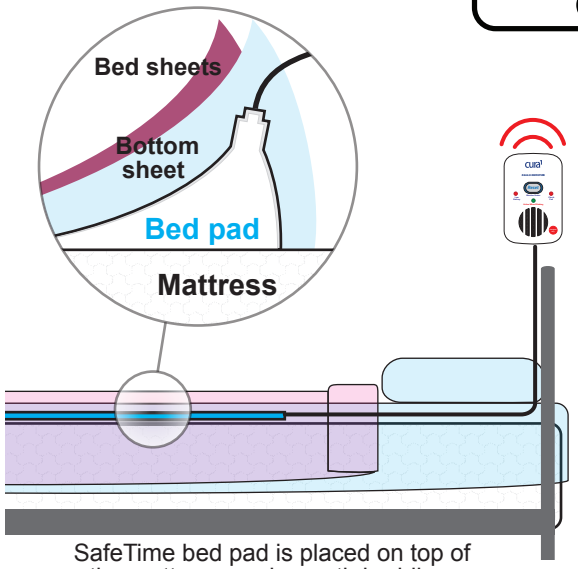

SafeTime bed pad is placed on top of the mattress, underneath bedding.

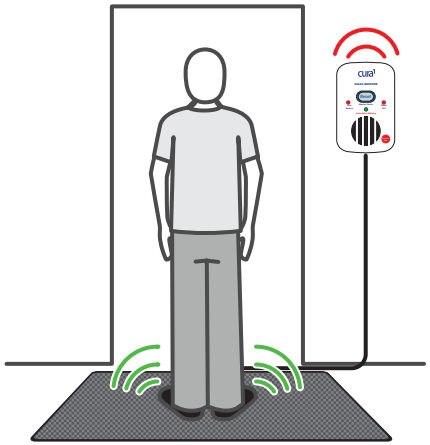

Premium floor mat is placed on floor in doorway or beside the bed.

Test falls monitor prior to every use.